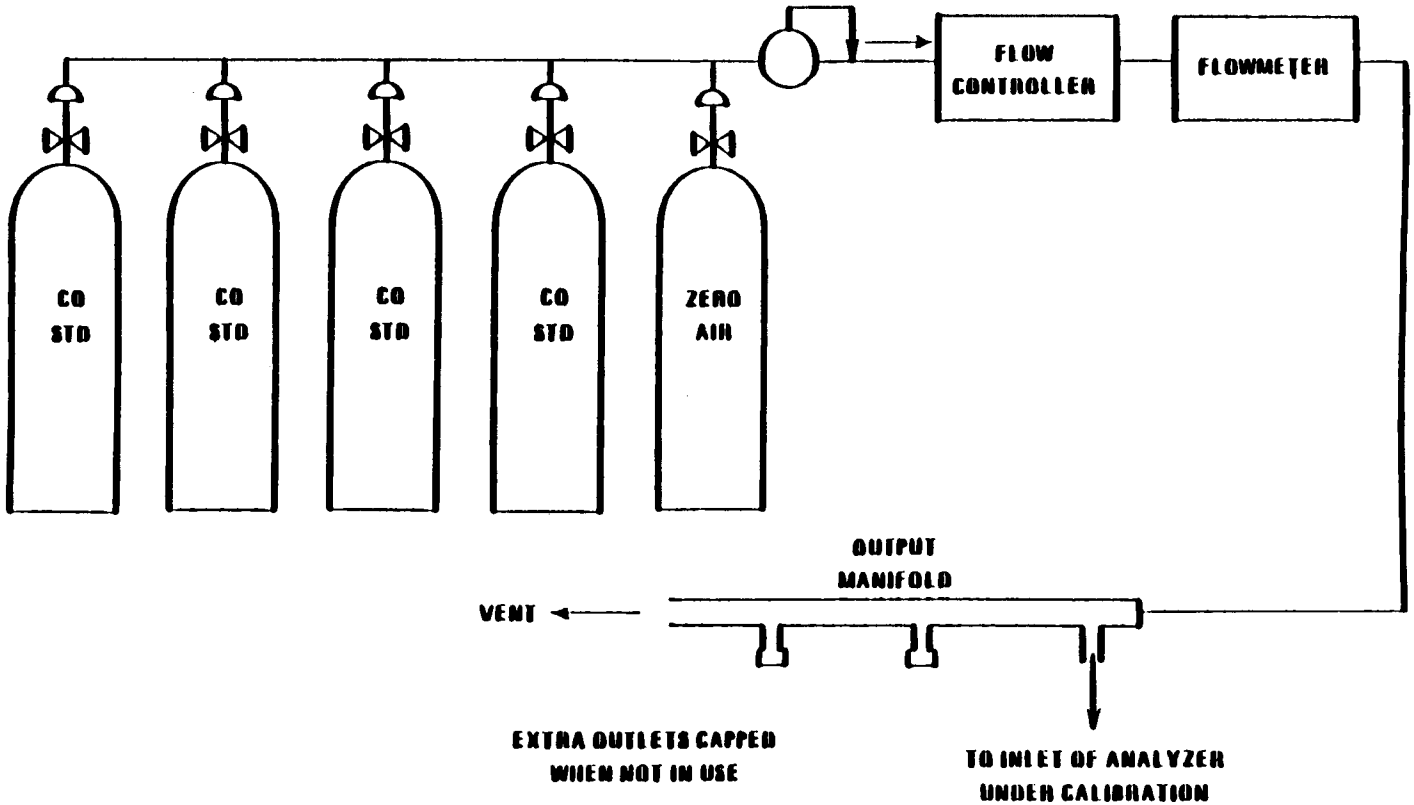

Figure 2. Multiple cylinder method for calibration of CO analyzers.